

ON THE CALIBRATION OF THE DMT MEMBRANE

by S. Marchetti, L'Aquila University, Italy <marchetti@flashnet.it>

INTERNAL TECHNICAL NOTE

(DRAFT 28 march 1999)

INTRODUCTION

This note summarizes various aspects related to the DMT membrane calibration and to the selection of DA, DB to be used in the calculations.

The "standard" instructions provided to operators for calibrating and exercising the membranes (reported in **Appendix 1** at the end of this note) are short and simple, and in general sufficient. However, in the years, many questions and problems have been raised by operators concerning unexpected situations, connected to soil type, membrane type, state of the blade etc. This note includes a collection of answers to such questions

Appendix 2 describes two recently developed auxiliary tools for facilitating the calibration /exercising operations.

IMPORTANCE OF ACCURATE DA, DB

Especially in soft soil, it is important to determine DA, DB accurately. Inaccurate DA, DB are virtually the only potential source of DMT error (the 1.1 mm displacement and the A, B pressures are practically error free). Attention must therefore be concentrated on DA, DB. Also, DA, DB are used to correct all A, B of a sounding, so any inaccuracy in DA, DB would propagate to all the data. Therefore all technicians involved with the DMT should be well familiar with the problems and their solutions discussed in this note.

The importance of DA, DB in soft soils derives from the fact that, in the extreme case of nearly liquid clays, or liquefiable sands, A and B are small numbers, just a bit higher than DA, DB. Since the correction involves differences between similar numbers, accurate DA, DB are necessary in such soils. (It is reminded that DA is recorded as a positive number, though the method of measuring it is via a suction).

DA, DB are, as a rule, measured before and after each sounding. Their average is subsequently used to correct all A, B. Clearly, if the variation is small, the average represents DA, DB reasonably well at all depths. If the variation is large, the average may be inadequate at some depths. In fact, in soft soils, the operator can be sure that a sounding has been successful only at the end of the test, if, checking DA, DB final, he finds that they are very similar to DA, DB initial.

In turn, a way of limiting undesired variations of DA, DB is to have DA, DB themselves small (ideally zero). Mechanical improvements in the years have reduced DA, DB in current blades to typically 0.15, 0.40 bar (after exercising). (1 bar = 100 Kpa).

Current recommendations (Eurocode '97) fix the following tolerances for DA, DB before testing: DA = 0.05 to 0.30 bar, DB = 0.05 to 0.80 bar. Higher values are appropriately not permitted, because they would unnecessarily increase possible DA, DB variations during the sounding. This is the reason why the "Minicalibrators" have a scale between 0.30 (suction) to 0.80 bar. Old (before 1990) blades have unfortunately higher DA, DB, and should be scrapped.

The reason of exercising new membranes is to stabilize their DA, DB (who vary mostly in the first cycles) prior to use in the soil, thereby reducing their variation during a sounding. Eurocode '97 limits the maximum variation of DA and DB before/after a sounding, to 0.25 bar.

In medium to stiff soils DA, DB are a small part of A and B, so small inaccuracies in DA, DB have negligible effect. In stiff soils one could (extreme hypothesis) even correct A and B using typical values of DA, DB (0.15 0.40 bar) rather than the measured DA, DB. From the substantial

viewpoint the Eurocode '97 prescriptions for DA, DB are too severe for a stiff soil, because the results would be correct anyway for all practical purposes. However using laxer tolerances is not advisable because it would induce the operator to a bad habit.

NOTE : The "membrane calibration" is not, strictly speaking, a calibration, since the term calibration is usually related to the scale of a measuring instrument. The membrane, instead, is a passive separator gas/soil and not a measuring instrument. Actually the membrane is a "tare" and the "calibration" is in reality a "tare determination". Such distinction will be ignored below.

SELECTING THE "AVERAGE" DA, DB TO BE USED IN THE CALCULATIONS

Selecting the average DA, DB is a step deserving the attention of the engineer. As a minimum, while performing the average, he will get a feeling of the entity of DA, DB and their variations during the sounding (a broad measure of the care exercised during the execution).

If the test has been regular (e.g. the membrane has not been overinflated, and the Eurocode '97 limits for DA, DB and their variations have not been exceeded), as it happens in most cases, the before/after values of DA, DB are very close, so that their arithmetic average is perfectly adequate (even though, if some rounding has to be done, it is advisable to choose the average on the low side. E.g. assume 0.14 as the average between 0.16 and 0.13).

The case of wider DA, DB variations is considered in a next paragraph.

INFLUENCE OF UNCERTAINTIES OF DA, DB ON THE INTERPRETED RESULTS

For the following considerations, the equations for interpreting Cu and Ed can be approximated as :

$$Cu = p_0 / 9 \qquad Ed = 34.7 [(B-A) - (DA+DB)]$$

Typical variations of DA during a sounding : from a few KPa to 20 KPa (20 KPa is an unusually high variation). Note that even such 20 KPa variation (corresponding to an uncertainty = distance from average = 10) would translate into an uncertainty in Cu of nearly 1 KPa, a very small quantity.

Typical variations of (DA+DB) during a sounding : from a few KPa to 30 KPa (30 KPa is an unusually high variation). Note that even such 30 KPa variation (uncertainty = 15) would translate into an uncertainty in Ed of nearly 5 bar, a quite small quantity.

In conclusion the resolution, even for unusually high DA, DB variations, are 1 KPa for Cu, 5 bar for Ed (or M). A more typical resolution is 0.5 KPa for Cu and 3 bar for Ed (or M). (All the above resolution figures should be intended preceded by the ± sign).

It may be noted that Cu is much less vulnerable than the moduli to uncertainties in DA, DB. Cu is derived essentially by A, and, as noted, uncertainties in DA very rarely translate into uncertainties in Cu higher than 1 Kpa. Hence even in situations of "bad DA, DB", Cu from DMT is instrumentally highly dependable.

SELECTING THE "AVERAGE" DA, DB IN CASE OF WIDE VARIATIONS

If DA or DB vary more than 0.25 bar during a sounding, the results, according to Eurocode '97 prescriptions, should be discarded and the sounding repeated. This is an appropriate clause for a standard. However, in many cases, the results can be salvaged, obtaining quite reasonable results, provided DA, DB are chosen with care. Unfortunately then, selecting DA, DB becomes subjective, which in general is undesirable and should be avoided.

For any useful purpose, this section offers guidance to perform judiciously such subjective DA, DB choice.

If the soil is stiff, the results are not much affected by DA, DB. Therefore, if using the arithmetic average of DA, DB, leads to a minimum value of Ed in the entire sounding say ≥ 25 bar, then DA, DB can be confirmed.

If the soil is soft, inaccurate or excessive DA, DB variations may give rise to several contradictions. A frequent contradiction, for instance, is the presence of many negative Ed (physically impossible). Such negative Ed will be noted by the operator when, after having entered the data in the computer, he prints the intermediate output, containing the input data and the Ed. In principle, in presence of several negative Ed, the results should be discarded. As an alternative, as mentioned, in many cases the data can still be salvaged by modifying judiciously DA, DB. In choosing the "adequate average" DA, DB, the following suggestions may be useful :

1. Verify if the negative Ed are only a few or many. In the first case check if A, B, at the depths of the negative Ed, were entered correctly. In case of suspect A,B enter 0,0 (interpreted by the computer as missing A,B at that depth).
2. If the Ed negative are many, (hence isolated typing errors are not the cause), all Ed can be lifted by reducing DA, DB. While reducing DA,DB keep in mind the following:
 - Typical average values of DA, DB are 0.15, 0.40.
 - Very seldom DA is outside the range 0.07-0.23 bar. Very often values of DA in the vicinity of 0.20 are directly reduced to 0.15 or 0.10.
 - Decrease DA, DB in a balanced (proportional) manner.
 - Keep reducing DA, DB until all Ed values are non-negative (or maybe 4-7 bar), by consulting each time the intermediate output.
3. In general, a "logical" average is better than the "arithmetic" average. For instance, in case of a combination of a soft layer and a hard layer, choose DA, DB closer to DA, DB that presumably were in effect in the soft layer, mostly in need of adequate DA, DB.

Another contradiction (the expert operator can use it to recognize a situation of bad DA, DB) is represented by pairs of A, B whose difference B-A is smaller than DA+DB (all positive numbers). E.g. if DA=0.15 and DB=0.40, B-A should not be less than 0.55. In fact the modulus Ed is proportional to the difference (B-A) - (DA+DB). Since DA, DB are nothing less than A and B in free air, the distance B-A, when the blade is in the soil, can only increase, but not decrease (negative modulus physically impossible). The same condition is expressed, in mathematical form, by the equation reported above for Ed. Hence B-A smaller than DA+DB signals some error either in A, B or in DA, DB. On the other hand, in water, or even in liquid mud, both B and A would increase with depth, but the difference would remain 0.55.

CASES WHEN DA, DB OF A NEW MEMBRANE ARE (RARELY) OUTSIDE TOLERANCE

When a new membrane is mounted on a current (after 1990) blade, DA, DB are, as a rule, within tolerance (even before exercising), i.e. $DA < 0.30$ bar and $DB < 0.80$ bar. Exercising the membrane further improves DA, DB, moving them towards the central values of the tolerance (say 0.15,0.40).

If, after mounting a new membrane, $DA > 0.30$ or $DB > 0.80$, the likely reason is that the blade is older than 1990. These blades are obsolete and should be scrapped. (Another good reason to scrap the old blades is that they were made of mild stainless steel, very vulnerable to damage and bending). Anyway even DA, DB of an old blade can be reduced within tolerance by the expedient of interposing an additional 0.15 gasket on top of the basic gasket.

Even in recent blades it has been found, exceptionally (when the geometrical tolerances combine most unfavorably), $DA > 0.30$ or $DB > 0.80$. In this case the remedy is to use a slightly

thicker neoprene gasket (say 0.97 mm rather than the usual 0.90 mm) or to add an additional 0.15 mm gasket on top of the basic gasket. This will reduce DA, DB within tolerance.

HOW DA, DB CAN GO OUT OF TOLERANCE AND HOW TO AVOID IT

In practice the only mechanism by which DA, DB can go out of tolerance is overinflation of the membrane (far) beyond the B position. Once overinflated, a membrane requires excessive suction to close (DA generally >0.30 bar), and even DB may be a suction.

It is possible that the soil, by pushing repeatedly against an overinflated membrane, will send it back below B. But then DA, DB final will differ considerably, in general, from the initial values.

For accuracy and productivity it is convenient to avoid the two causes of membrane overinflation.

The first cause is a trivial one, i.e. omitting deflation after the B-signal. This may happen to an inexperienced operator, but he will learn quickly.

A more serious reason can be the absence of the B-signal (an electrical malfunctioning). This inconvenience is discussed in the next section.

ABSENCE OF THE B-SIGNAL


Such absence is due to the lack of contact at the B-position, in turn due to dirt/ grains/ tissue at the points of electrical contact, namely below the sensing disk or at the bases of the small steel cylinders (see arrows in the figure below).

If the absence of B starts suddenly in the middle of a sounding, the operator has no way of being aware of this inconvenience, and finds himself in a puzzling situation, since he does not know if the high pressure he is reaching is due to an unexpectedly stronger layer or to the absence of B-signal. In such cases a prudent step may be to deflate and take a second chance by advancing the tip 10 cm, rather than the usual 20 cm, and repeating A, B. (Then the operator must advance the tip only 10 cm to recoup the right sequence).

The obvious remedy to the absence of the B-signal is to keep well clean the electrical contact points, blowing each of the involved pieces with compressed air. There is no need to do the cleaning periodically, but only after a damage allowing dirt inside the blade.

A recommended check (before starting a sounding) useful for reducing the risk of absence of B reading during a sounding, is the following. At the beginning of the test (i.e. at calibration), push-pull the syringe i.e. repeat DA, DB 10 or 20 times, to make sure that the A-signal and B-signal are sharp.

Another rare cause of absence of B-signal may be the lack of contact between the sensing disk and its seating, i.e. the disk not reaching the bottom of the seating. This, in turn, may be due to inadequate gripping force of the pvc lining on the sensing disk. The correct gripping should correspond to an extraction force of the sensing disk of at least 2 or 3 Kg. If the coupling becomes loose (disk too free to move) then the gripping force should be re-increased. One quick fix can be the addition, while reinstalling the disk, of a small piece of plastic sheet laterally (NOT on the bottom).

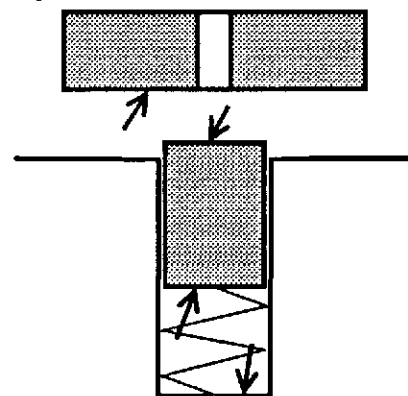

TYPES OF MEMBRANES AVAILABLE

This information updates previous information contained in various manuals or papers.

Since 1990 one type of membrane is by far the mostly frequently used. This type is the "high strength" (or "hard") membrane 0.20 mm thick.

Such choice is a consequence of the improvements introduced in all blades after 1990 in the shape of the "hub" receiving the membranes. Such improvements have led to DA, DB, with hard membranes, lower than old blades with soft membranes. Thus the combination "new blade + hard membranes" has low DA, DB, and, at the same time, substantially increased damage resistance. Therefore the old soft membranes, though still available, are rarely used.

Another valid type of membrane is also available. The material is the same as the "high strength" membranes, but the thickness is 0.25 mm, further increasing damage resistance. Fortunately DA, DB of the 0.25 membranes are only 15-20% higher than for the 0.20 mm membranes, i.e. their typical DA, DB are say 0.18, 0.55. Hence their possible variation during a sounding is larger by a similar percentage. Thus the typical resolution for the 0.25 mm membranes may be 0.8 KPa for Cu and 5 bar for Ed (or M). Since the difference in resolution (0.8 vs 0.5 Kpa for Cu and 5 vs 3 bar for Ed) is quite small, then the 0.25 mm thickness may be preferable when testing in soils that may cut the membrane.

NOTE : In order to distinguish soft/hard membranes, examine the outer rim. If the rim is perfectly flat, the membranes are soft. If the rim has "waves", the membranes are hard.

HOW TO HANDLE THE ZERO OFFSET OF THE GAGE (Z_m)

Ideally, the zero offset of the pressure gage (Z_m = reading of the gage of the front panel of DMT when the vent valve is open) should be zero (in most DMT pressure gages Z_m can be regulated and set to zero). However small deviations, properly considered, are influential on accuracy.

The rest of this paragraph will consider the general case of a gage having a non-zero Z_m .

In order to handle Z_m correctly, it is necessary to recognize first which one of the following 2 cases applies :

- **Case 1** : the same gage is used for reading DA, DB and all subsequent A and B
- **Case 2** : DA, DB are determined using a separate accurate vacuumometer (with typically its zero offset =0). Then all A, B are read by means of the gage of the DMT.

Since the introduction of the dual gage front panel (approximately 1990), **Case 1** is by far the most common, since the low scale gage permits to read DA, DB with fair accuracy.

In **Case 1** Z_m should be recorded as zero even if Z_m is not zero. In fact not only all A, B, but also DA, DB are affected by Z_m , so that the Z_m correction is already accounted for in DA, DB (this compensation can be derived readily from the algebra of the correction formulae for A and B). In conclusion today's operators have to write "zero" for Z_m in the field form. If the operator prefers, for correctness of documentation, he can write the real Z_m . But in any case later in the computer Z_m must be entered as $Z_m=0$ (entering the real Z_m would result in applying twice the correction to A and B).

By contrast, in **Case 2** (the today unusual case when the old single-gage panel is used) the Z_m that operators have to write in the field form is the real Z_m of the front panel gage. Similarly, the Z_m to be entered later in the computer must be the real Z_m . This because originally the formulae were developed assuming that DA, DB were exact (being measured by a separate accurate vacuumometer), and only A and B needed the correction.

BIBLIOGRAPHY

Details on membrane calibration and selection of DA, DB can also be found in the following two references, though, of course, many changes since have been updated in this document.

- Marchetti, S. & Crapps, D.K. 1981. Flat Dilatometer Manual. Internal Report of G.P.E. Inc. (in particular p.4.1)
- Schmertmann, J.H. 1988. Guidelines for Using the CPT, CPTU and Marchetti DMT for Geotechnical Design. U.S. Dept. of Transportation, Federal Highway Administration, Office of Research and Special Studies. Report No. FHWA-PA-87-024+84-24, Vol. 3-4. (In particular Vol. 3 - DMT Test Methods And Data Reduction pp. 2.16-2.22)

APPENDIX 1

"STANDARD" OPERATOR'S INSTRUCTIONS CONCERNING : MEMBRANE CALIBRATION AND EXERCISING PROCEDURE

CALIBRATION

The membrane calibration (determining DA, DB) can be performed in two configurations :

1. The first configuration (**blade accessible**) is adopted for example at the beginning of a sounding, when the blade is still in the hands of the operator. The operator will then use the short calibration cable, or the short calibration connector (attached to a clamp on the carrying case).
2. The second configuration (**blade not readily accessible**) is used when the blade is under the penetrometer, and is connected to the control box with cables of normal length (say 20 to 30 m).

Calibration using the short calibration connector (blade accessible)

Insert the syringe quickconnector into the socket "syringe" in the front panel

Detach the "short calibration connector" from the clamp in the carrying case and :

- (a) Attach one end to the blade to be calibrated"
- (b) Plug the quickconnector into the socket "dilatometer" in the front panel.
- (c) Connect the electrical jack to the socket "ground" in the front panel

Set piston of the syringe approximately half way (when in need of sucking or expel surplus air, open/ then close the fast-vent-valve).

Pull back (almost fully) the piston of the syringe, then slowly release it and read DA.

Push slowly the piston of the syringe and read DB. (If necessary to charge/discharge the syringe, open/ then close the fast-vent-valve).

Repeat the DA, DB determination a few times to be sure, then write their values.

Calibration with the blade under the penetrometer (blade not readily accessible).

The connections are the same as during current testing. Thus the blade is connected to the control box by a tubing say 20 or 30 m long, while the ground cable connects the control box to the rods.

Set piston of the syringe approximately half way and proceed as indicated in the previous configuration. The only difference is that, due to the length of the DMT tubings, the response of the pressure gages to the syringe is not immediate (there is some time lag). Therefore, in that configuration, DA, DB must be taken slowly.

NOTES

During calibration, the valve "general" should be closed, to avoid communication with the high-pressure portion of the circuit. Better still, the gas tank should be disconnected and the entire high-pressure portion vented. As an additional precaution, close also the micrometer valve, not needed for the calibration.

Generally DA, DB of a blade are checked in the office (e.g. by the Minicalibrator) and written on a sticker on the blade. Once in the field, there could be small differences between DA and DB on the sticker and DA, DB taken before testing. The DA, DB to consider are those taken, just before testing, with the same control box used to take all the A, B readings.

EXERCISING PROCEDURE

After having mounted a new membrane, the membrane needs to be "exercised" in order to stabilize DA, DB. The exercising operation simply consists in pressurizing the blade in free air at 4-5 bar. This pressurization can be performed in the same configuration as when testing, or, more conveniently, using an auxiliary tool, the "exercise syringe", permitting to perform handily the exercising operation, without need to use the gas tank, the control box and a tubing.


The "exercise syringe" is directly screwed (as a screwdriver) on the rear of the blade. Note that the syringe has a **START** mark and an **END** mark. Before connecting the syringe to the blade, the piston should be at the **START** position, then the syringe can be screwed to the blade.

When pushing the piston of the syringe from **START** to **END**, the air pressure will reach 4 to 5 bar, which is the pressure needed for the exercising (the force is approximately 25 Kg, or 250 Newton).

The exercising pressure can be applied only once, or, equally well, 2 or 3 times.

If the exercising is performed with the blade vertical submerged in a bucket of water, it is possible to verify blade airtightness.

After exercising, insure that DA, DB are in tolerance : DA=0.05 to 0.30 (typically 0.15), DB=0.05 to 0.80 b

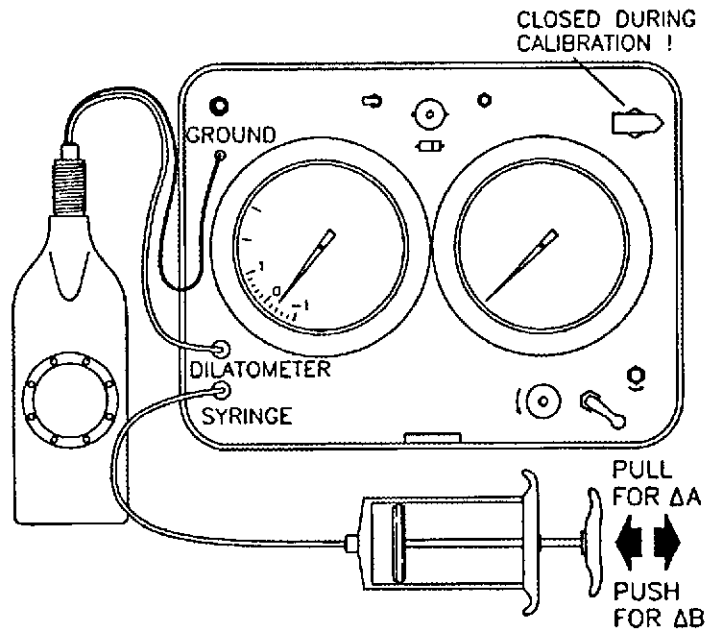

Connections during calibration in case the blade is easily accessible

APPENDIX 2

TWO AUXILIARY TOOLS FOR FACILITATING THE CALIBRATION AND THE EXERCISING OPERATIONS : THE MINICALIBRATOR AND THE EXERCISE SYRINGE

THE MINICALIBRATOR

The Minicalibrator is an auxiliary tool permitting to perform handily the calibration of a membrane (determine DA, DB) and to verify the proper functioning of a blade (regular on/off switching of the signal), without need of deploying the regular control box.

Characteristics of the Minicalibrator:

- It is small (20 cm long) and light (200 grams), and is able by itself (without control box, cables, ground cable) to check DA, DB of a blade.
- It is equipped with a pressure gage that is small, but has a scale spanning the full tolerance range (-30 to 80 KPa), and therefore is very accurate.
- It is equipped with a small buzzer and a battery that will last for years. Uses one 1/2 AA 3V battery, terminating with wires (easily found in computer shops).
- It is directly screwed (as a screwdriver) on the rear of the blade.

It fulfills **fast and conveniently** the following tasks :

- Check DA, DB after a blade has just been revised.
- Check DA, DB and run a general functioning check of a blade in the office before moving to a site.
- Check if DA, DB have reached regular values after installing / exercising a new membrane.
- Check handily in a hotel room, after a day of field work, if the blades are working properly. If DA, DB are outside the green scale of the gage, the membrane has to be replaced. (Note that blades older than 1990 may have DA, DB too high. Anyway DA, DB of a new membrane in an old blade can still be reduced within tolerance by interposing an additional 0.15 gasket on top of the basic gasket).
- Permits to field supervisors to verify quickly if the blades in use at the site are working properly and DA, DB are in tolerance

"Cleanliness" check

The Minicalibrator also permits to verify if the inside of the blade, below the sensing disk, is free from dirt or pieces of tissue or fabric. For this check, the operator applies 10 or 20 push-pull cycles and note if the signal inversions are sharp. If they are "hesitant", the operator should remove the membrane and clean or blow off dirt from the electrical contact points.

NOTE

- DA, DB of a real test, as a rule, must be taken - and written in the data sheet - just before (and after) a sounding using the **same** control box used for performing the sounding. Hence DA, DB taken previously with the Minicalibrator have to be considered as indicative. Nevertheless, in most cases, the differences are very small.
- Due to the lack of tubing, the response of the gage of the Minicalibrator to the pressures applied by the syringe is immediate. This immediate response should not induce the operator to forget that, when he takes DA, DB with the usual 20 or 30 m DMT tubing, there is some time lag, and therefore, in the configuration with real tubings, he must take DA, DB slowly.

THE MINICALIBRATOR



THE EXERCISE SYRINGE

The "exercise syringe" is an auxiliary tool permitting to perform handily the exercising operation, without need to use the gas tank, the control box and a tubing.

The exercising operation is performed whenever a new membrane is mounted. The scope is to stabilize DA, DB. The operation consists in pressurizing the blade in free air at 4-5 bar.

The "exercise syringe" is directly screwed (as a screwdriver) on the rear of the blade. Note that the syringe has a **START** mark and an **END** mark. Before connecting the syringe to the blade, the piston should be at the **START** position, then the syringe can be screwed to the blade.


When pushing the piston of the syringe from **START** to **END**, the air pressure will reach 4 to 5 bar, which is the pressure needed for the exercising (the force is approximately 25 Kg, or 250 Newton).

The exercising pressure can be applied only once, or, equally well, 2 or 3 times.

If the exercising is performed with the blade vertical submerged in a bucket of water, it is possible to verify blade airtightness.

After exercising, insure that DA, DB are in tolerance : DA=0.05 to 0.30 (typically 0.15), DB= 0.05 to 0.80 bar (typically 0.40).

THE EXERCISE SYRINGE

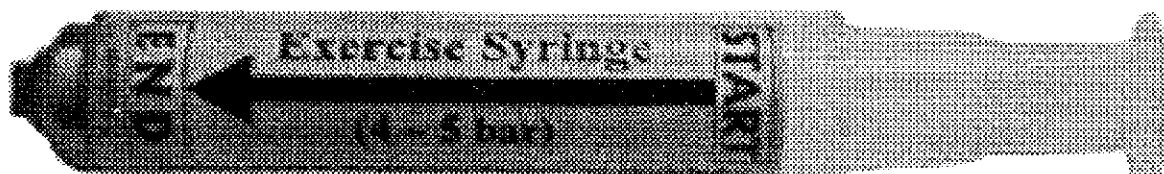

SUMMARY OF VARIOUS ASPECTS RELATED TO MEMBRANE CALIBRATION

IMPORTANCE OF ACCURATE DA, DB

Especially in soft soil, it is important to determine DA, DB accurately. Inaccurate DA, DB are virtually the only potential source of DMT error (1.1 mm displacement and A, B pressures are practically error free). It is therefore worthwhile to concentrate attention on DA, DB. Also, DA, DB are used to correct all A, B of a sounding, so any inaccuracy in DA, DB would propagate to all data.

The importance of accurate DA, DB in soft soils derives from the fact that, in the extreme case of nearly liquid soils, A, B are small numbers, just a bit higher than DA, DB. The correction is essentially a difference between similar numbers, hence accurate DA, DB are necessary in such soils. (It is reminded that DA is recorded as a positive number, though it is a suction).

DA, DB are, as a rule, measured before and after each sounding. Their average is subsequently used to correct A, Bs. Clearly, if the variation is small, the average represents DA, DB reasonably well at all depths. If the variation is large, the average may be inadequate at some depths. In fact, in soft soils, the operator can be sure that a sounding has been successful only at the end of the test, if, checking DA, DB final, he finds that they are very similar to DA, DB initial.

In turn, to limit the potential variations of DA, DB, they have to be as small as possible (ideally zero). Mechanical improvements in the years have reduced DA, DB in current blades to typically 0.15, 0.40 (after exercising to 5 bar).

Current recommendations (Eurocode '97) fix the following tolerances for DA, DB before testing : DA = 0.05 to 0.30 bar, DB = 0.05 to 0.80 bar. Higher values are appropriately not permitted, because they would unnecessarily increase possible DA, DB variations during the sounding. This is the reason why the "minicalibrators" have a scale between 0.30 (suction) to 0.80 bar. Old (before 1990) blades have unfortunately higher DA, DB, and should be scrapped.

The reason of exercising new membranes is to stabilize their DA, DB (who vary most in the first cycles) prior to use in soil, thereby reducing their variation during a sounding. Eurocode '97 limits the maximum variation of DA and DB before/after sounding, to 0.25bar.

In medium to stiff soils DA, DB are a small part of A and B, so small inaccuracies in DA, DB have negligible effect. In stiff soils one could even correct A and B using typical values of DA, DB (0.15 0.40 bar) rather than the measured DA, DB. From the substantial viewpoint the above prescription for DA, DB are too severe for a stiff soil, because the results are practically correct anyway. However using laxer tolerances is not advisable because it would induce the operator to a bad habit.

SELECTING THE "AVERAGE" DA, DB TO BE USED IN THE CALCULATIONS

Selecting the average DA, DB is a step deserving the attention of the engineer. Moreover, while performing the average, the engineer will become aware of the entity of DA, DB variation during the sounding.

If the test has been regular (e.g. the membrane has not been overinflated, and the above limits of DA, DB and their variations have not been exceeded - as it happens in most cases), the before/after values of DA, DB are so close that their arithmetic average is perfectly adequate (even then, however, if there is some number to be rounded, choose the average on the low side. E.g. assume 0.14 as the average between 0.16 and 0.13).

INFLUENCE OF UNCERTAINTIES OF DA, DAB ON THE INTERPRETED RESULTS

For the considerations that follow, the correlations for obtaining Cu and Ed can be rounded to $Cu=1/10 Po$, $Ed= 34.7 * (B-A) -(DA, DB)$.

Typical variations of DA during a sounding are in a range from a few KPa to 20 KPa (a limit rarely attained). Note that even a relatively high variation of 20 KPa (=uncertainty of 10) translates into an uncertainty in Cu of nearly 1 KPa, a very small quantity.

Typical (DA+DB) variations : from a few KPa to 30 KPa (a limit rarely attained). Note that even a relatively high variations of 30 KPa (=uncertainty of 15) translates into an uncertainty in Cu of nearly 5 bar, a quite small quantity.

In conclusion the resolution, for relatively high Da, DB variations, are 1kPa for Cu, 5 bar for the moduli. A more typical resolution is 0.5 kPa for Cu and 3 bar for moduli.

HOW TO SELECT THE "AVERAGE" DA, DB IN CASE OF WIDE VARIATIONS

If DA or DB vary more than 0.25 bar during a sounding, according to the prescriptions, the results should be discarded and the sounding repeated. This is an appropriate clause for a standard. However in many cases the results can be salvaged, obtaining very reasonable results, provided DA, DB are chosen with care. Unfortunately then, selecting DA, DB becomes subjective, and this is undesirable and should be avoided.

For any useful purpose this section offers guidance to perform in a judicious way such subjective DA, DB choice.

First, if the soil is stiff, the results are not much affected by DA, DB. Therefore, if entering the arithmetic DA, DB average, the minimum value of Ed in the sounding is say 25 bar, then DA, DB can be confirmed.

Inaccurate or too variable DA or DB in a soft soil will result in several contradictions.

For instance it is a contradiction to find, at any given depth, a difference B-A is smaller than DA+DB (all positive numbers). E.g. if DA=0.15 and DB=0.40, B-A should not be less than 0.60. In fact the modulus Ed is proportional to the difference B-A. Since DA, DB are nothing less than A and B in free air, the distance B-A, when the blade is in

the soil can only increase, but not decrease (negative modulus physically meaningless). Hence the above circumstance signals some error or in A, B or in DA, DB.

When reducing the data by computer, normally the program first prints a draft output including the input data and Ed. Again, if many negative Ed show up, this means that DA, DB are too high. (This will not happen if the above tolerances were respected). As an alternative to discarding the sounding, in many cases the data can still be salvaged by modifying DA, DB as follows: *****To be reworked up to the end of this section*****

- a. Verify if the negative Ed are only a few or many. In the first case check if A, B, at the anomalous depths, were entered correctly at some depths. If this is the case, enter the right A, B at those depths.
- b. If a. has not eliminated the Ed negative, and there are still many Ed negative (systematic), DA, DB introduced have to be decreased. Then decrease DA, DB keeping in mind the following:
 - Typical values of DA, DB are 0.15, 0.40.
 - Decrease in a balanced (proportional) manner DA, DB
 - Keep reducing DA, DB until all Ed values in the draft output are zero (or maybe 4-7 bar)

Logical average .If something wrong choose an average reflecting especially the value in the soft part of the profile

WHAT TO DO WHEN DA, DB OF A NEW MEMBRANE ARE (RARELY) OUTSIDE TOLERANCE

When a new membrane is mounted on a current (after 1990) blade, DA, DB are, as a rule, within tolerance (even before exercising), i.e. $DA < 0.30$ bar and $DB < 0.80$ bar. Exercising the membrane further improves the corrections, approaching them to the central values of the tolerance (say 0.15, 0.40).

If, after mounting a new membrane, $DA > 0.30$ or $DB > 1$, the likely reasons is that the blade is older than 1990. These blades are obsolete should be scrapped.

NOTE : Old blades, being made of mild stainless steel, are also very vulnerable to damage and bending. Anyway DA, DB of a new membrane in an old blade can still be reduced within tolerance by interposing an additional 0.15 gasket on top of the basic gasket.

It has been found in recent blades, exceptionally (when the geometrical tolerances combine most unfavorably),

$DA > 0.30$ or $DB > 1$. In this case the remedy is to use a slightly thicker neoprene gasket (say 0.97 mm rather than the usual 0.90 mm) or to add an additional 0.15 mm gasket on top of the basic gasket. This will reduce DA, DB within tolerance.

HOW DA, DB CAN GO OUT OF TOLERANCE AND HOW TO AVOID IT

In practice the only mechanism that can bring DA, DB out of tolerance, during a sounding, is overinflation of the membrane (far) beyond the B position. An overinflated membrane requires excessive suction to close (DA generally > 0.30 bar), and often even DB may be a suction.

In some cases the soil, pushing repeatedly against an overinflated membrane, sends it back below B. But then DA, DB final will be considerably different, in general, from the initial values.

For accuracy and productivity it is convenient to pay attention to the two causes of membrane overinflation, in order to avoid them.

The first cause is a trivial one, i.e. omitting deflation after the B-signal. This may happen to inexperienced operators, but they will learn quickly.

A more serious reason can be the absence of the B-signal (an electrical malfunctioning). Such absence is due to dirt/ grains/ tissue at the points of electrical contact, namely below the sensing disk or at the bases of the small steel cylinders. If the absence of B starts suddenly in the middle of a sounding, the operator gets no warning, and finds himself in a puzzling situation, since he does not know if the high pressure he is reaching is due to a stronger layer or to absence of B-signal. In such cases he can deflate and have a second chance by advancing the tip 10 cm, rather than the usual 20 cm, and repeating A, B. Then he will advance the tip 10 cm to follow the right sequence.

The obvious remedy to absence of B-signal is to keep well clean the electrical contact points. There is no need to do the cleaning periodically, but only after a damage allowing dirt inside the blade.

A recommended check useful for reducing the risk of absence of B reading during a sounding is the following. At the beginning of the test (i.e. at calibration), push-pull the syringe i.e. repeat DA, DB 10 or 20 times, to be sure that the A-signal and B-signal are sharp.

TYPES OF MEMBRANES AVAILABLE

This information updates previous information contained in various manuals or papers.

Since 1990 one type of membrane is by far the mostly frequently used. This type is the "high strength" (or "hard") membrane 0.20 mm thick.

Such choice is a consequence of the improvements introduced in all blades after 1990 in the shape of the "hub" receiving the membranes. Such improvements have led to DA, DB, with hard membranes, lower than old blades with soft membranes. Thus the combination "new blade + hard membranes" has low DA, DB, and, at the same time, substantially increased damage resistance. Therefore the old soft membranes have been abandoned.

An alternative type of membrane is also available. The material is the same as the "high strength" membranes, but the thickness is 0.25 mm, further increasing damage resistance. Since DA, DB are only 15-20% higher than for the 0.20 thickness, the 0.25 mm membranes could be preferred when testing frequently in hard soils, since the accuracy loss is very small.